

Supplement:

Table S1 Bulk soils properties and distribution of fraction weights, C and N in aggregate-size fractions.

Site	Horizon	Depth	C	N	pH	MWD	Gravels in LM	W5	W4	W3	W2	W1	C5	C4	C3	C2	C1	N5	N4	N3	N2	N1
		cm	%	%		mm	%	%	%	%	%	%	%	%	%	%	%	%	%	%	%	%
Wet (Cajamarca)																						
LS1	A _{h1}	20	12.51	1.10	6.17	4.22	0.00	29.2	18.6	43.5	7.9	0.7	11.94	11.73	12.25	13.59	12.23	1.06	1.05	1.06	1.24	1.07
	A _{h2}	37	7.20	0.64	6.07	6.42	0.75	51.6	20.2	26.2	2.0	0.0	6.67	8.39	8.05	9.37	10.58	0.61	0.74	0.72	0.83	0.87
	B _t	57	3.73	0.40	6.22	7.99	18.91	68.9	17.4	13.2	0.5	0.0	3.96	4.53	5.19	7.38	6.91	0.40	0.46	0.50	0.68	0.64
LS2	A _{h1}	14	14.84	1.21	5.25	5.33	0.29	41.1	20.4	25.2	8.9	4.1	14.22	14.25	14.66	15.42	11.64	1.15	1.18	1.18	1.27	0.95
	A _{h2}	40	12.65	1.01	5.50	4.80	0.00	34.4	24.0	29.5	9.2	2.9	12.15	12.46	12.60	13.58	10.58	0.95	1.00	1.01	1.11	0.87
	A _{h3}	55	7.67	0.60	5.98	6.37	0.00	50.7	22.3	23.4	3.4	0.2	7.44	8.24	8.34	9.26	7.22	0.57	0.65	0.67	0.73	0.58
	B _{tg}	66	2.41	0.24	6.49	8.72	18.43	77.1	15.6	7.1	0.2	0.0	2.11	2.44	2.90	3.69	2.67	0.22	0.24	0.27	0.33	0.24
LS3	A _p	12	12.63	1.01	5.57	5.64	0.00	44.8	16.3	31.4	6.0	1.3	12.21	11.66	12.43	13.25	12.40	0.99	0.97	0.99	1.10	1.05
	A _{h2}	37	7.47	0.57	6.42	4.97	0.00	36.1	22.4	34.3	6.1	1.0	7.52	7.32	7.17	7.78	8.25	0.57	0.57	0.55	0.63	0.65
	A _{h3}	47	4.59	0.34	6.84	7.66	0.14	65.3	18.2	14.7	1.6	0.3	4.55	5.12	4.81	5.19	5.99	0.32	0.37	0.35	0.40	0.45
	B _{tg}	60	2.37	0.20	6.97	8.30	0.62	73.7	11.6	13.6	1.1	0.0	1.98	2.98	3.17	3.59	4.27	0.18	0.23	0.25	0.27	0.34
AS1	A _p	20	3.30	0.28	4.99	3.76	11.16	29.2	7.9	34.0	23.2	5.6	3.77	3.70	2.32	4.48	6.78	0.30	0.30	0.18	0.39	0.60
	A _{h2}	45	3.46	0.29	4.90	4.00	4.96	29.3	14.8	34.1	17.0	4.8	3.83	3.79	2.82	4.19	7.48	0.32	0.32	0.25	0.36	0.65
	A _{h3}	68	2.97	0.26	5.00	3.80	17.00	26.4	16.1	39.3	14.0	4.2	3.06	2.83	2.21	3.47	5.93	0.25	0.24	0.19	0.30	0.55
AS2	A _p	20	9.24	0.67	5.03	2.89	9.14	18.4	13.9	39.2	21.1	7.0	9.82	9.70	7.53	8.77	14.28	0.68	0.69	0.52	0.63	1.01
	A _{h2}	45	7.38	0.52	4.96	2.93	18.10	17.7	15.9	42.8	19.3	4.3	8.01	7.52	6.81	9.24	12.68	0.56	0.52	0.47	0.68	0.88
AS3	A _{h1}	15	9.38	0.66	5.54	3.79	9.26	24.4	23.9	32.8	14.1	4.4	10.83	9.83	8.34	10.43	12.28	0.78	0.68	0.58	0.74	0.91
	A _{h2}	35	5.90	0.43	5.26	3.08	43.10	18.6	19.4	37.7	17.3	6.9	7.15	5.67	5.16	7.95	10.01	0.52	0.42	0.37	0.60	0.72
Dry (Carhuaz)																						
LS1	A _{h1}	22	3.62	0.33	5.21	3.72	8.95	21.8	28.9	35.6	9.8	3.6	4.35	3.59	3.87	3.27	3.85	0.39	0.34	0.34	0.32	0.37
	A _{h2}	42	2.34	0.25	5.11	5.99	7.18	48.8	16.9	23.7	8.1	2.5	2.15	2.33	2.39	2.43	2.60	0.26	0.27	0.27	0.27	0.28
	B _t	56	1.99	0.24	5.02	7.35	10.48	63.4	13.9	17.9	4.0	0.9	1.82	1.96	1.95	2.05	2.61	0.27	0.25	0.26	0.25	0.30
LS2	A _{h1}	21	2.95	0.32	5.85	6.18	9.53	49.1	22.0	22.5	5.0	1.3	2.86	3.07	3.11	3.01	3.82	0.33	0.34	0.35	0.34	0.44
	A _{h2}	34	1.39	0.20	5.58	6.72	7.13	55.3	19.3	20.5	3.7	1.1	1.22	1.35	1.34	1.45	1.92	0.21	0.21	0.22	0.20	0.27
	B _{tg}	54	0.77	0.17	5.74	7.70	0.00	66.2	17.0	13.7	2.3	0.8	0.64	0.71	0.72	0.94	1.01	0.17	0.18	0.17	0.19	0.20
LS3	A _{h1}	21	4.29	0.40	5.02	5.00	6.89	37.2	21.2	30.0	9.0	2.4	3.98	3.77	4.69	4.67	4.70	0.39	0.37	0.44	0.45	0.48
	A _{h2}	42	2.62	0.27	4.95	4.43	15.21	29.9	25.4	34.6	7.7	2.4	2.79	2.60	2.71	2.58	3.48	0.31	0.29	0.28	0.26	0.38
	A _{h3}	62	2.05	0.24	5.11	4.52	11.89	28.6	33.6	30.2	5.8	1.8	2.03	2.02	2.05	2.11	2.70	0.25	0.26	0.24	0.26	0.31
	B _{tg}	73	1.69	0.22	5.25	4.44	22.56	28.3	30.7	34.1	5.4	1.4	1.72	1.74	1.74	2.09	2.27	0.23	0.23	0.22	0.25	0.30
AS1	A _{h1}	19	7.27	0.54	5.49	1.62	57.95	7.3	9.2	43.1	27.5	12.8	7.18	6.97	5.62	7.69	8.97	0.46	0.51	0.43	0.63	0.76
	A _{h2}	44	6.66	0.48	5.26	2.43	44.45	14.4	12.6	38.8	21.2	12.9	6.32	5.25	4.41	6.26	8.93	0.47	0.40	0.33	0.49	0.70
AS2	A _{h1}	10	4.62	0.32	5.63	2.03	55.76	8.3	15.3	51.6	20.8	3.6	5.83	5.41	5.96	5.74	6.45	0.40	0.38	0.38	0.42	0.50
	AC	15	1.98	0.14	5.82	1.20	80.25	1.0	9.6	64.9	18.5	6.0	2.69	2.52	1.93	2.80	4.69	0.20	0.19	0.14	0.20	0.35
	2A _{bh}	60	4.40	0.31	5.24	2.90	31.46	16.3	16.8	50.9	13.6	2.3	5.40	4.31	4.10	5.66	6.41	0.38	0.30	0.29	0.42	0.49
AS3	A _{h1}	19	4.81	0.32	4.83	1.90	33.58	10.9	4.2	50.2	24.2	10.0	6.27	5.60	5.63	4.29	8.96	0.42	0.33	0.35	0.31	0.65
	A _{h2}	50	4.40	0.30	4.78	1.01	77.88	1.6	6.7	49.8	27.9	13.7	7.11	5.17	6.98	5.04	8.24	0.47	0.35	0.43	0.37	0.63

LS: limestone soil, AS: acid igneous rock soil, Wet: the wet site, Dry: the dry site, MWD: mean weight diameter, LM: large macroaggregates (>2 mm), W: weight percentage, C: organic carbon content, N: nitrogen content, -5: fractions >5 mm, -4: fraction 2-5 mm, -3: fraction 0.25-2 mm, -2: fraction 0.063-0.25 mm, -1: fraction <0.063 mm.

Table S2 SOC concentrations and bulk densities every 10 cm.

Depth	SOC content	Bulk density	Bulk density corrected for stones	Depth	SOC content	Bulk density	Bulk density corrected for stones	Depth	SOC content	Bulk density	Bulk density corrected for stones
cm	%	g cm ⁻¹	g cm ⁻¹	cm	%	g cm ⁻¹	g cm ⁻¹	cm	%	g cm ⁻¹	g cm ⁻¹
Wet-LS1				Wet-LS2				Wet-LS3			
10	14.69	0.51	0.51	10	13.72	0.75	0.75	10	11.33	0.71	0.71
20	13.46	0.58	0.58	20	14.41	0.78	0.78	20	9.56	0.78	0.78
30	10.18	0.76	0.75	30	11.43	0.84	0.84	30	9.33	0.76	0.75
40	6.48	0.89	0.88	40	8.99	0.87	0.87	40	6.22	0.89	0.89
50	5.29	1.02	1.01	50	6.45	0.99	0.98	50	4.31	1.06	1.05
60	3.33	1.14	1.10	60	3.28	1.19	0.70	60	2.25	1.28	1.27
Average	8.91	0.82	0.81	Average	8.47	0.97	0.89	Average	7.17	0.91	0.91
Wet-AS1				Wet-AS2				Wet-AS3			
10	3.84	1.16	1.09	10	8.97	0.78	0.77	10	9.57	0.73	0.71
20	3.34	1.15	1.13	20	8.81	0.75	0.75	20	7.43	0.80	0.72
30	3.93	1.09	1.09	30	7.37	0.85	0.78	30	5.70	0.87	0.82
40	4.11	0.99	0.99	40	4.97	0.83	0.65	40	5.14	0.84	0.77
50	3.23	1.16	0.91	50	0.95	1.05	0.50	50	0.55	1.16	1.09
60	2.74	1.08	1.01								
70	1.67	1.05	0.85								
Average	3.27	1.10	1.01	Average	6.21	0.85	0.69	Average	5.68	0.88	0.82
Dry-LS1				Dry-LS2				Dry-LS3			
10	4.95	0.96	0.94	10	4.08	1.08	0.97	10	5.05	0.95	0.92
20	2.56	1.01	0.97	20	2.14	1.07	1.02	20	3.34	1.08	1.05
30	2.32	0.99	0.96	30	1.51	1.16	1.09	30	2.78	1.09	1.05
40	2.17	1.08	1.08	40	0.99	1.29	1.21	40	2.38	1.07	1.03
50	1.96	1.04	1.01	50	0.57	1.28	1.28	50	2.11	1.11	1.08
60	1.47	1.22	1.19	60	0.66	1.25	1.25	60	2.09	1.16	1.09
Average	2.57	1.05	1.03	Average	1.66	1.19	1.14	Average	2.78	1.09	1.05
Dry-AS1				Dry-AS2				Dry-AS3			
10	6.88	0.74	0.48	10	5.19	0.73	0.68	10	4.88	0.99	0.85
20	5.46	0.87	0.64	20	2.78	1.13	0.89	20	4.77	0.70	0.62
30	5.37	0.78	0.74	30	3.48	1.04	0.74	30	4.88	0.72	0.69
40	2.29	0.96	0.75	40	4.31	0.81	0.73	40	5.45	0.78	0.69
50	0.91	1.21	1.18	50	4.08	0.84	0.78	50	4.48	1.09	0.77
60	0.98	1.28	1.25	60	4.59	1.03	0.77				
				70	0.51	1.59	1.25				
Average	3.65	0.97	0.84	Average	3.56	1.03	0.83	Average	4.89	0.86	0.72

Wet: the wet site, Dry: the dry site, LS: limestone soil, AS: acidic igneous bedrock soils

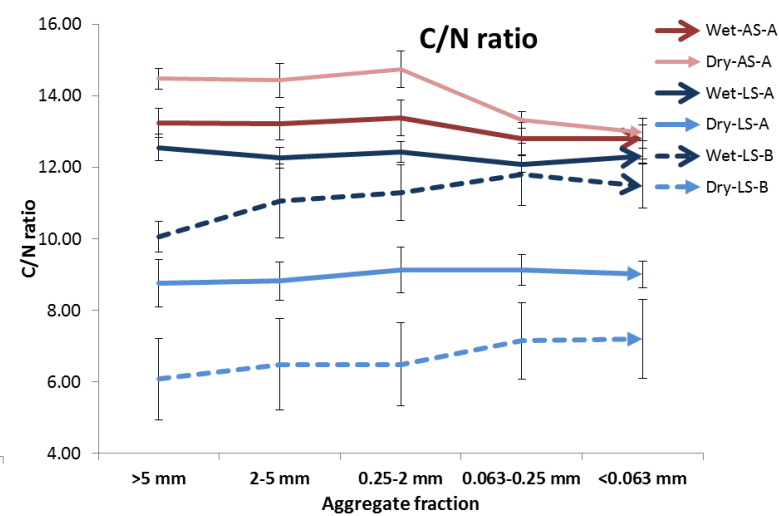
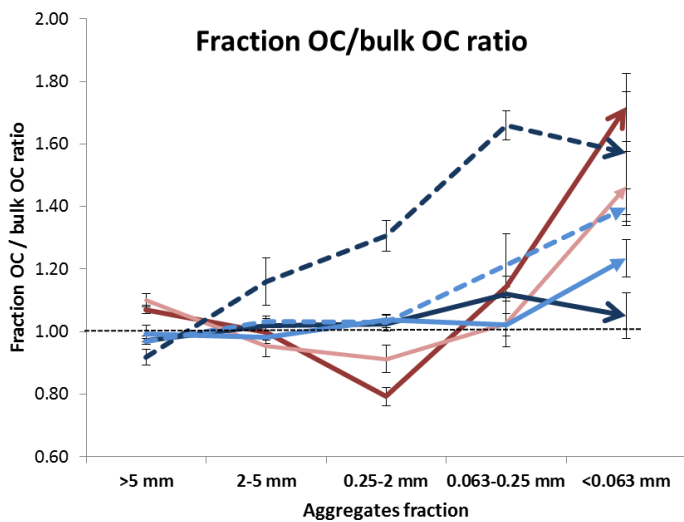
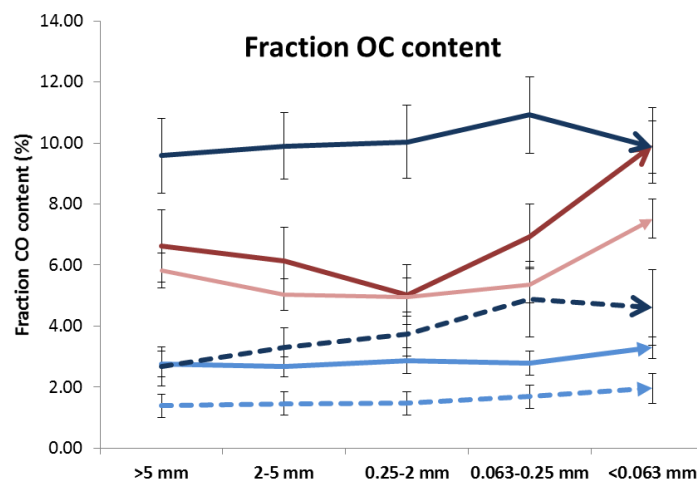
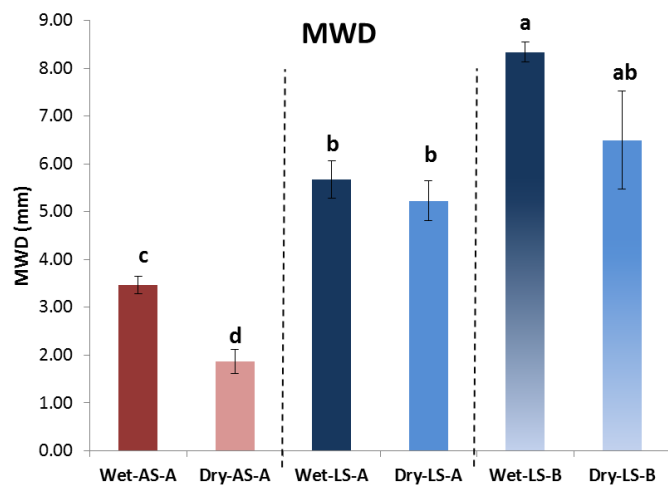


Fig. S1 Mean weight diameters (MWD) of soil horizons and properties of aggregate size fractions. Arrows indicate decreasing aggregate sizes. Wet: the wet site, Dry: the dry site, LS: limestone soil, AS: acid igneous rock soil, A: A horizons, B: B horizons, fraction OC content: organic carbon contents of aggregate-size fractions.

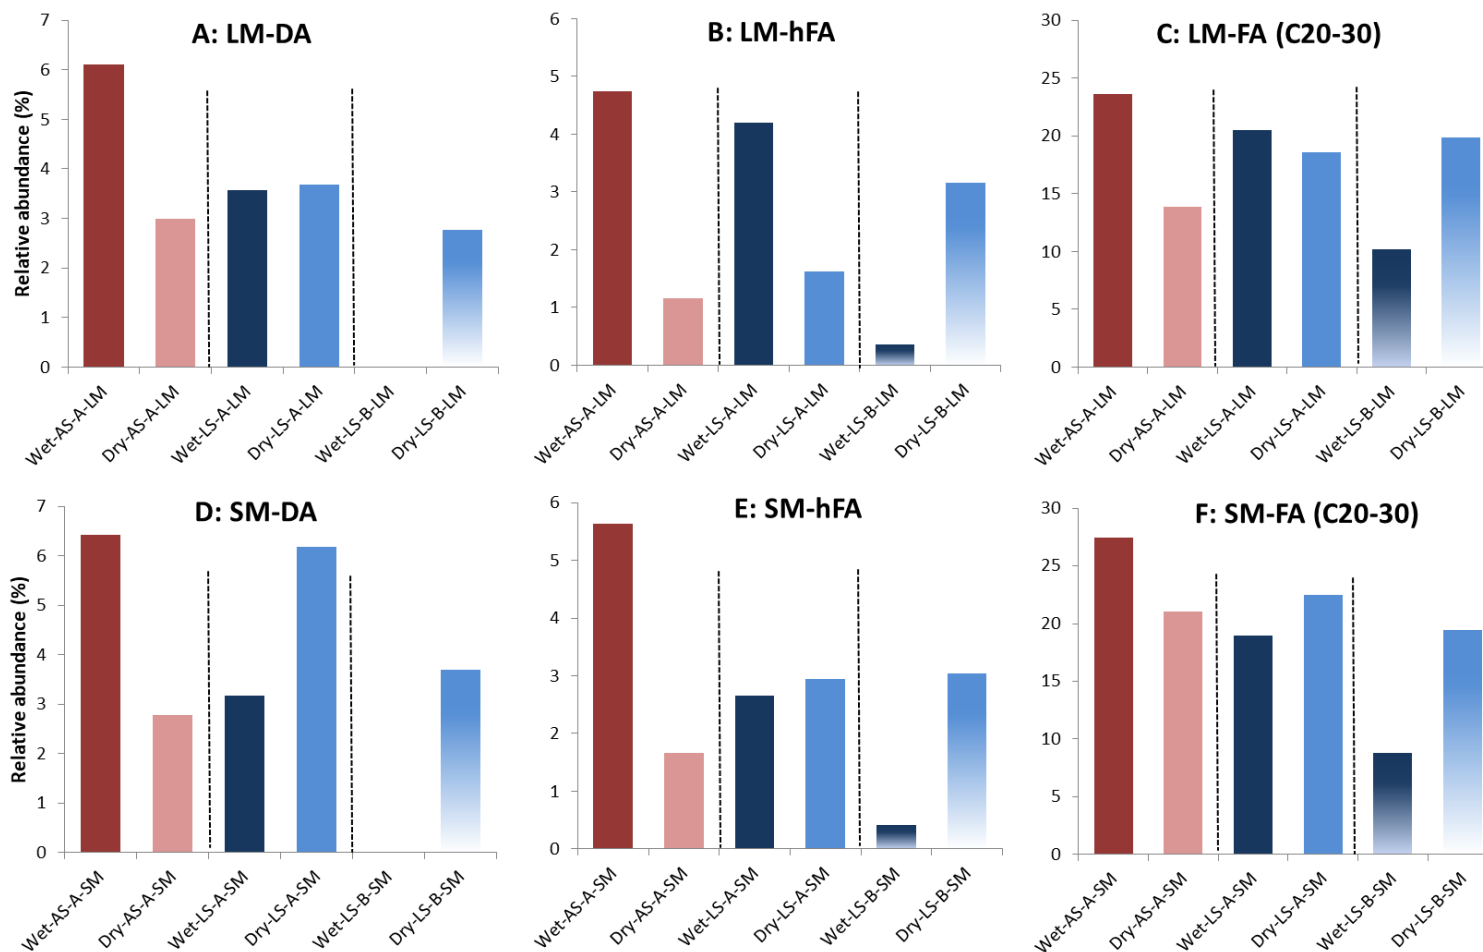


Fig. S2 Relative abundances of α , ω -dioic acids (DA), hydroxyl alkanolic acid (hFA) and long-chain fatty acids (FA) in aggregate fractions before the incubation. Pyrolysis-gas chromatography / mass spectrometry (GC/MS) was applied to estimate the molecular composition of the soil organic matter. Briefly, milled soil samples were hydrolyzed and methylated using tetra-methyl-ammonium hydroxide (25 % in water). Afterward, a Curie-point pyrolyzer was used for sample pyrolysis. Helium was used as the carrier gas. Initial temperature was kept at 40 °C for 1 min, followed by heating at the rate of 7 °C min⁻¹ until 320 °C sustaining for 15 min. The products of the pyrolysis were analyzed by the GC/MS system. Relative abundance of each compound was calculated as the peak area of the compound divided by the sum of peak areas of all identified compounds. Wet: the wet site, Dry: the dry site, LS: limestone soil, AS: acid igneous rock soil, A: A horizons, B: B horizons, LM: large macroaggregates (>2 mm), SM: small macroaggregates (0.25-2 mm).